

Assurance of energy handling capability in accordance with ISO 21254-3

Measurement Report

Sample: R16075-1

Request from: Central Laser Facility
STFC Rutherford Appleton Laboratory
Chilton, Didcot, OX11 0QX,
United Kingdom

Contact person: Mariastefania De Vido

Testing institute: Lidaris Ltd.
Saulėtekio al. 10,
LT-10223, Vilnius,
Lithuania, EU

Tester/date: L. Vigricitė / 2017-05-05

Specimen

Name of sample: R16075-1

Type of specimen: Glass

Storage, cleaning: Plastic box, wrapped in paper for optics

Test specification

Fundamental harmonic of pulsed Nd:YAG InnoLas Laser: SpitLight Hybrid laser ($\lambda = 1064$ nm, linear polarization, pulse duration 10.0 ns), $\lambda/2$ plate combined with additional polarizer attenuator, online scattered light damage detection, offline inspection of damage detection using Nomarski microscopy (100x).

Laser parameters used for testing

Wavelength: 1064 nm
Angle of incidence: 0 deg.
Polarisation state: linear
Pulse repetition frequency: 100 Hz
Spatial beam profile in target plane: TEM₀₀
Longitudinal beam profile: Single longitudinal mode (SLM)
Beam diameter in target plane ($1/e^2$): $(976.4 \pm 42.7) \mu\text{m}$ (average from 500 pulses)
Pulse duration (FWHM): $(10.0 \pm 0.3) \text{ ns}$ (average from 1000 pulses)

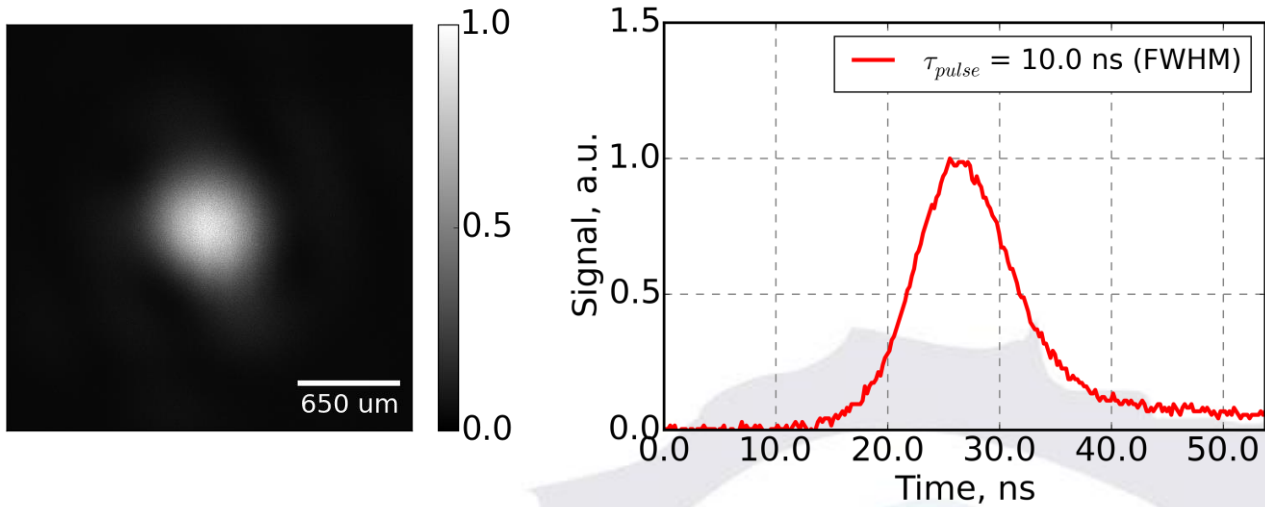


Fig. 1. Spatial beam profile in target plane (left) and temporal pulse profile (right).

Test procedure:

Assurance levels:
 Number of sites per assurance level:
 Number of shots per site:
 Tested area:
 Arrangement of test sites:
 Damage detection:
 Storage of the specimen:

 Test environment:
 Cleaning:

Assurance of energy handling capability

3.5, 5, 7.5 J/cm²
 449
 1000
 1 cm²
 Hexagon, equally spaced, 50% overlap (Fig 2.)
 Post-test inspection, Nomarski microscopy
 Manufacturer's packaging,
 normal laboratory conditions
 Industrial environment
 Dust blown off with clean air

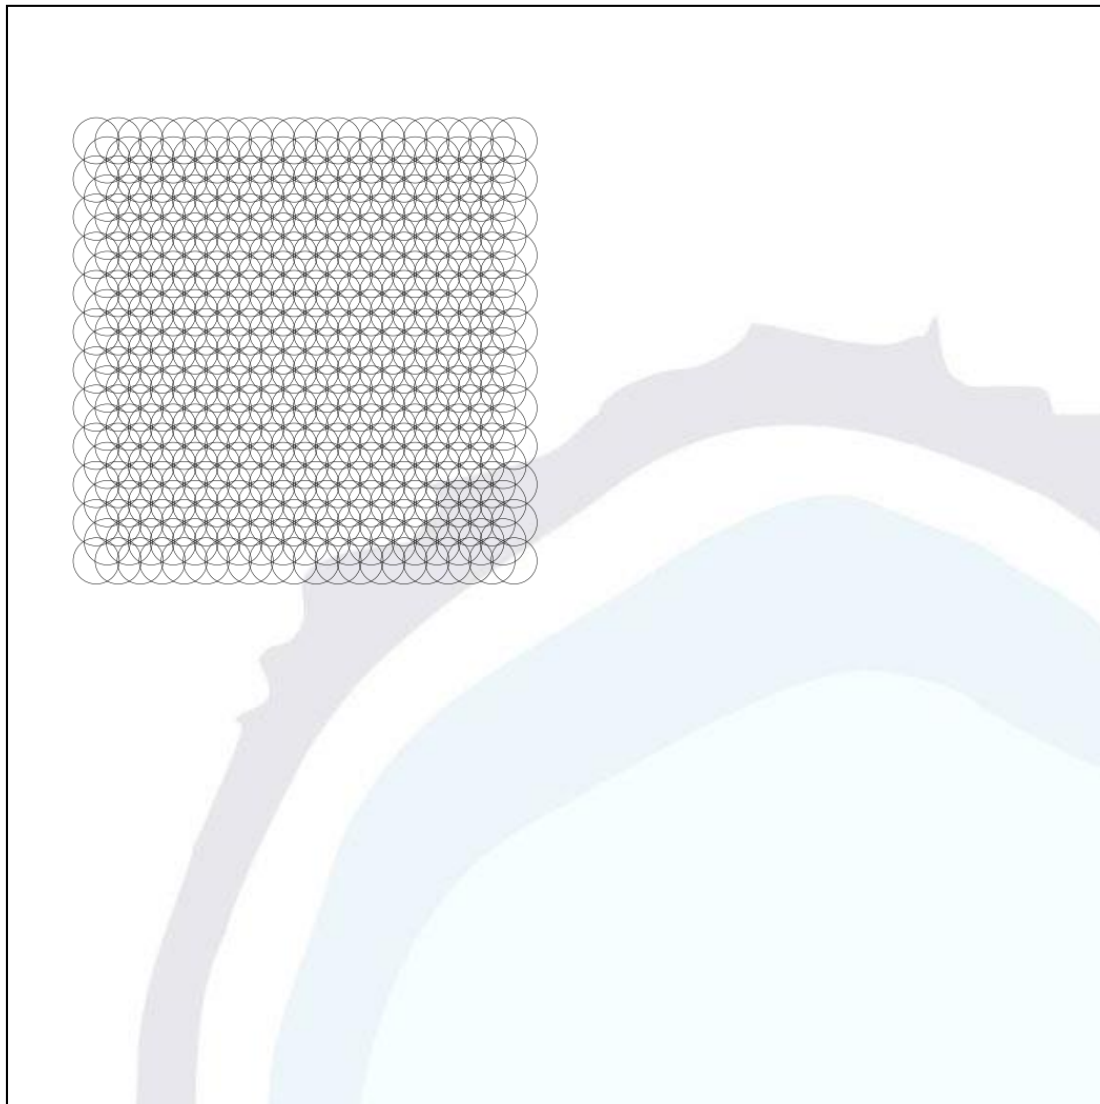


Fig. 2. Arrangement of test sites

Test result:

Table 1. Test results for sample R16075-1.

Assurance level	Result
$3.5 \pm 0.5 \text{ J/cm}^2$	Passed
$5.0 \pm 0.9 \text{ J/cm}^2$	Passed
$7.5 \pm 1.3 \text{ J/cm}^2$	Passed